


JRC CRL - FCM Database / GC-MS

Sample Name: Acetic acid, vinyl ester
Solvent: Ethanol
Concentration: 100 µg/mL

Date: 19/09/2005
CAS: 000108-05-4
PM ref: 10120 [U.R.N. M032]

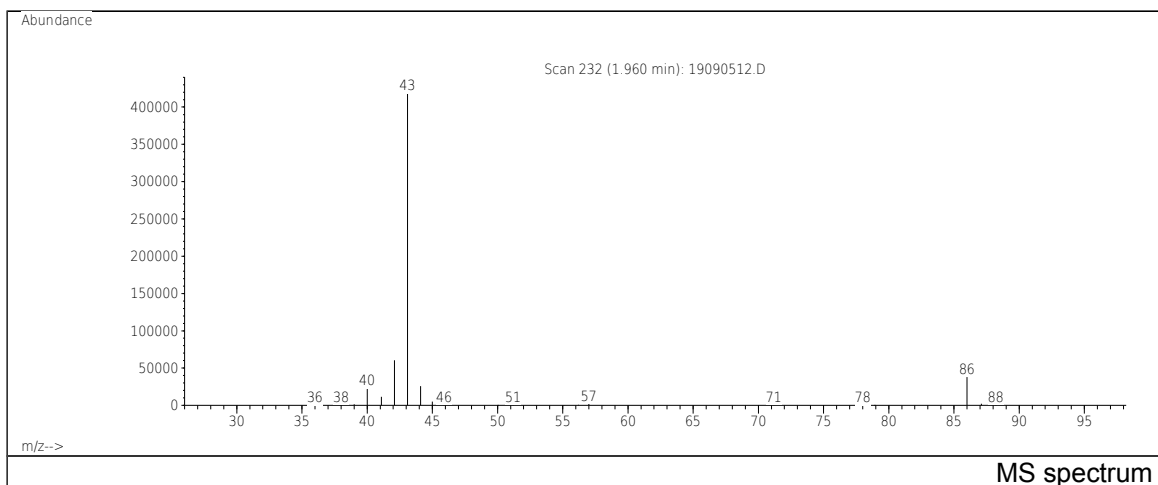

m/z	Abundance	Ion Intensity %	m/z	Abundance	Ion Intensity %
38.10	409,0	0,12	52.90	303,0	0,09
39.10	753,0	0,22	56.00	781,0	0,23
40.00	22536,0	6,55	57.10	1758,0	0,51
41.10	9435,0	2,74	58.00	358,0	0,10
42.10	45216,0	13,14	86.10	27872,0	8,10
43.10	344000,0	100,00	87.00	1794,0	0,52
44.10	22488,0	6,54	88.20	324,0	0,09
45.10	3986,0	1,16			

Spectrometer: HEWLETT PACKARD GC/MS 6890/5973
Inlet system: capillary GC/MS
Scan Range: 40-700 amu
Source temperature: 230 °C

Flow: 1.2 mL/min
Column: DB 17-HT (30 m x 0.25 mm x 0.15 µm)
Programme temperature: 40 °C (3 min); 20 °C/min
(350 °C); 350 °C (20 min)