


JRC CRL - FCM Database / GC-MS

Sample Name: Methanol
Solvent: -
Concentration: 100 µg/mL

Date: 17/01/2005
CAS: 000067-56-1
PM ref: 21550 [U,R.N. M123]

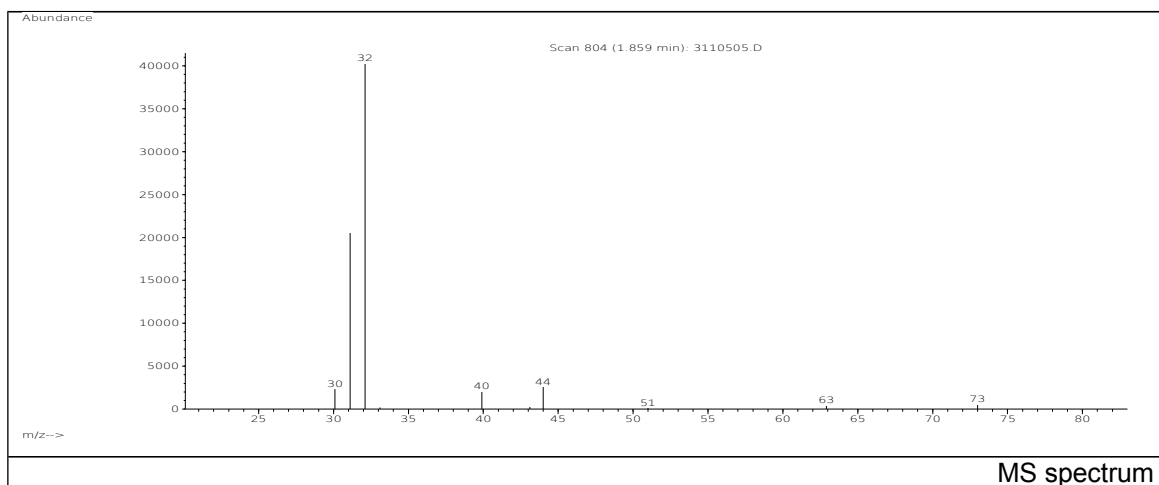

m/z	Abundance	Ion Intensity %	m/z	Abundance	Ion Intensity %
30.10	2345,0	5,65	62.90	427,0	1,03
31.10	20528,0	49,48	73.00	551,0	1,33
32.10	41488,0	100,00			
33,10	196.0	0,47			
39,90	2048.0	4,94			
43,10	243.0	0,59			
44,00	2635.0	6,35			
51,00	174.0	0,42			

Spectrometer: HEWLETT PACKARD GC/MS 6890/5973
Inlet system: capillary GC/MS
Scan Range: 30-700 amu
Source temperature: 230 °C

Flow: 1.2 mL/min
Column: DB 17-HT (30 m x 0.25 mm x 0.15 µm)
Programme temperature: 40 – 300 °C (20 °C/min)