
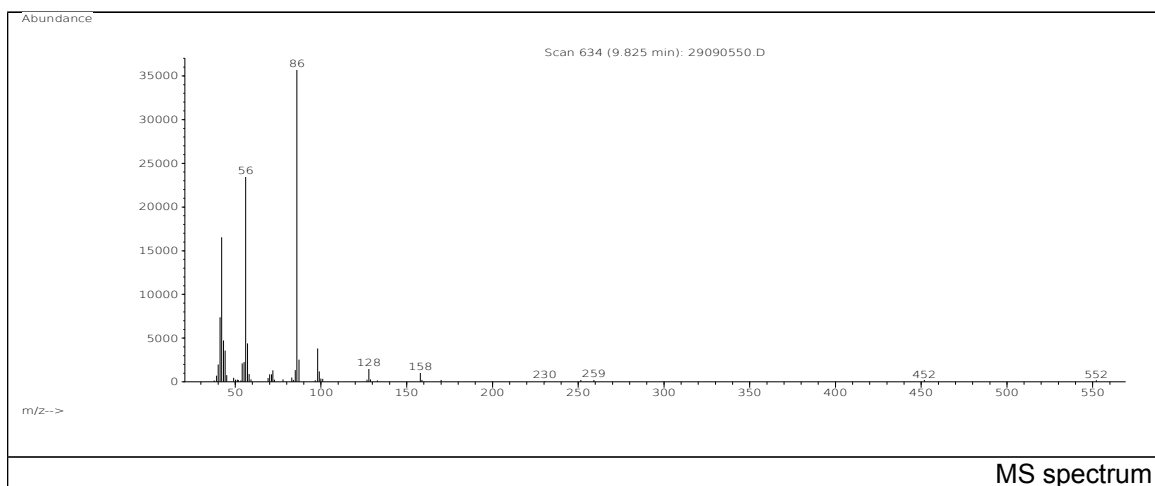


JRC CRL - FCM Database / GC-MS

Sample Name: 2-aminoethanol
Solvent: Methanol
Concentration: 100 µg/mL

Date: 29/09/2005
CAS: 000141-43-5
PM ref: 22337 [U.R.N. M186]

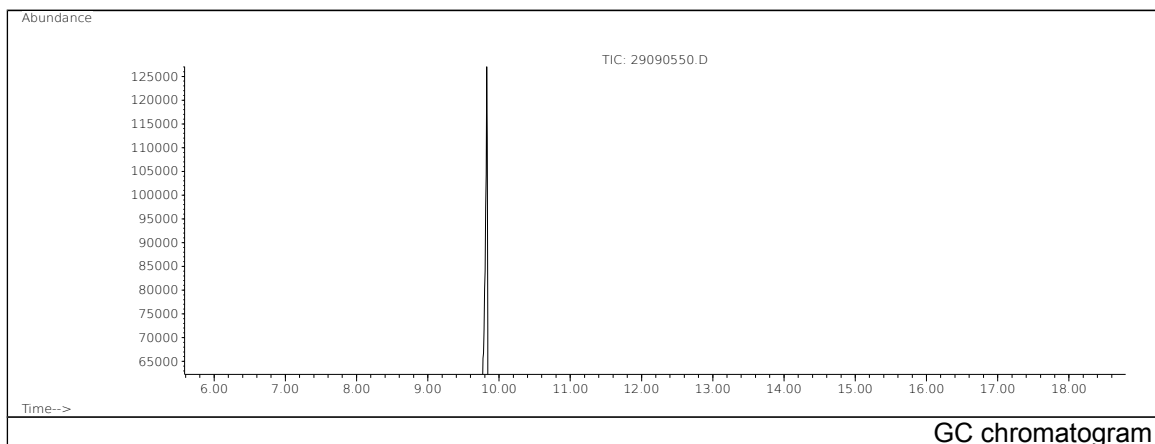

m/z	Abundance	Ion Intensity %	m/z	Abundance	Ion Intensity %
40.00	1998,0	5,40	57.10	4390,0	11,85
41.10	7391,0	19,96	72.00	1325,0	3,58
42.10	16528,0	44,63	85.00	1349,0	3,64
43.20	4728,0	12,77	86.00	37032,0	100,00
44.10	3591,0	9,70	87.10	2550,0	6,89
54.00	2106,0	5,69	98.10	3809,0	10,29
55.10	2275,0	6,14	127.90	1546,0	4,17
56.10	23512,0	63,49			

Spectrometer: HEWLETT PACKARD GC/MS 6890/5973
Inlet system: capillary GC/MS
Scan Range: 40-700 amu
Source temperature: 230 °C

Flow: 1.2 mL/min
Column: DB 17-HT (30 m x 0.25 mm x 0.15 µm)
Programme temperature: 40 °C (3 min); 20 °C/min
(350 °C); 350 °C (20 min)