
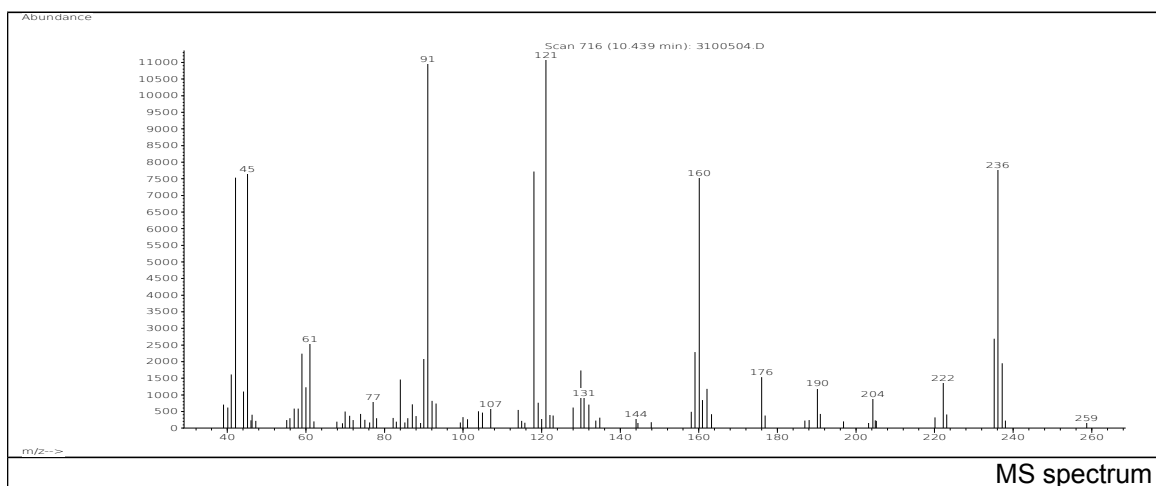


JRC CRL - FCM Database / GC-MS

Sample Name: 3-Aminopropyltriethoxysilane
Solvent: Methanoll
Concentration: 100 µg/mL

Date: 03/10/2005
CAS: 000919-30-2
PM ref: 12786 [U.R.N. M214]

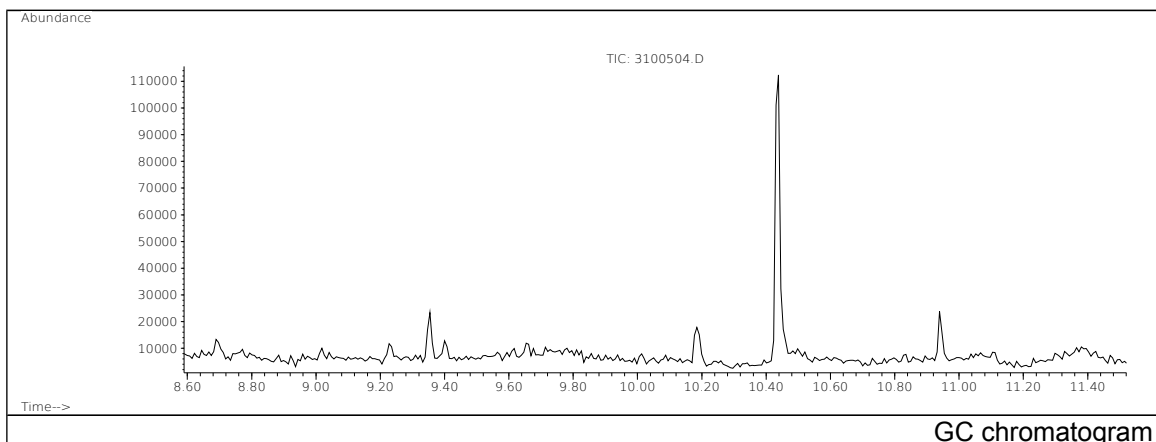

m/z	Abundance	Ion Intensity %	m/z	Abundance	Ion Intensity %
41.00	1617,0	14,23	121.10	11362,0	100,00
42.10	7533,0	66,30	130.00	1739,0	15,31
45.10	7665,0	67,46	159.00	2287,0	20,13
59.00	2240,0	19,71	160.10	7533,0	66,30
61.00	2539,0	22,35	235.20	2690,0	23,68
90.00	2081,0	18,32	236.10	7786,0	68,53
91.00	10957,0	96,44	237.20	1954,0	17,20
118.00	7716,0	67,91			

Spectrometer: HEWLETT PACKARD GC/MS 6890/5973
Inlet system: capillary GC/MS
Scan Range: 40-700 amu
Source temperature: 230 °C

Flow: 1.2 mL/min
Column: DB 17-HT (30 m x 0.25 mm x 0.15 µm)
Programme temperature: 40 °C (3 min); 20 °C/min
(350 °C); 350 °C (20 min)